


# Methanol Delivery System

for EPA Method 5035

sample smart

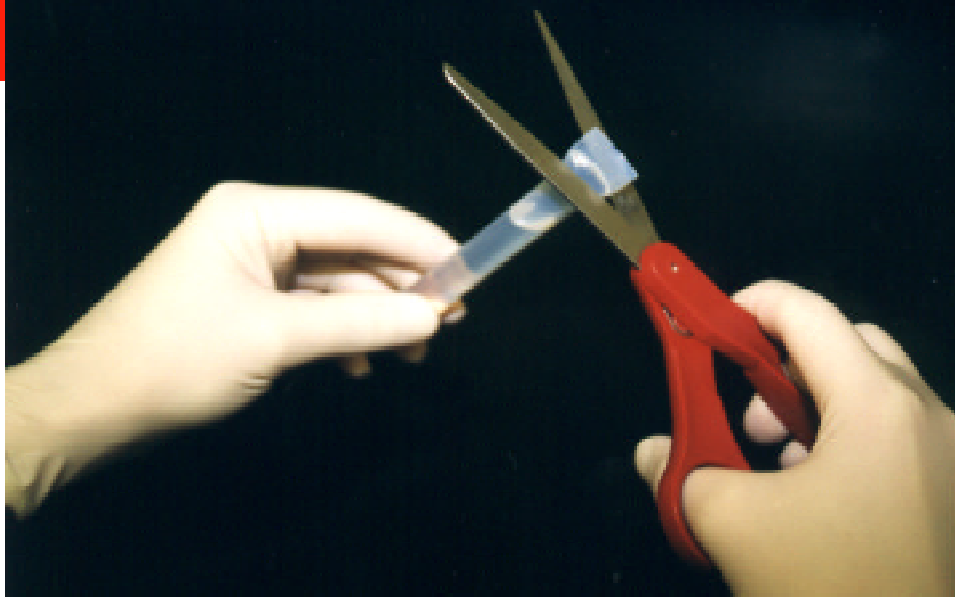

EPA Method 5035 specifies that methanol vials used in field preservation must be reweighed in the field to verify methanol weight prior to sample collection. This is not typically practical during field sampling. With **o2si's samplesmart** methanol delivery system, the need to weigh methanol in the field is eliminated through the introduction of pre-measured methanol from a uniquely sealed Teflon tube. The **samplesmart** methanol delivery system prevents weight loss and provides the sampler with an easy method of preservation without the need for weighing, thus decreasing collection times. Furthermore, surrogates can be added to the **samplesmart** methanol delivery system by **o2si** so that samples arrive at the laboratory ready for analysis.

## Provides Significant Cost Savings:

- Eliminates Field Weighing
- Decreases Collection Times
- Increases Productivity
- Eliminates Methanol Loss
- Introduces Surrogates During Sampling



Contact Daniel R. Biggerstaff, Ph.D.  
(843) 763-4884  
P.O. Box 30712 • Charleston, SC 29417  
[www.o2si.com](http://www.o2si.com)

**o2si** is an ISO 9001 certified company.

