

METHOD 8330

NITROAROMATICS AND NITRAMINES BY HIGH
PERFORMANCE LIQUID CHROMATOGRAPHY (HPLC)

1.0 SCOPE AND APPLICATION

1.1 Method 8330 is intended for the trace analysis of explosives residues by high performance liquid chromatography using a UV detector. This method is used to determine the concentration of the following compounds in a water, soil, or sediment matrix:

Compound	Abbreviation	CAS No ^a
Octahydro-1,3,5,7-tetranitro-1,3,5,7-tetrazocine	HMX	2691-41-0
Hexahydro-1,3,5-trinitro-1,3,5-triazine	RDX	121-82-4
1,3,5-Trinitrobenzene	1,3,5-TNB	99-35-4
1,3-Dinitrobenzene	1,3-DNB	99-65-0
Methyl-2,4,6-trinitrophenylnitramine	Tetryl	479-45-8
Nitrobenzene	NB	98-95-3
2,4,6-Trinitrotoluene	2,4,6-TNT	118-96-7
4-Amino-2,6-dinitrotoluene	4-Am-DNT	1946-51-0
2-Amino-4, 6-dinitrotoluene	2-Am-DNT	355-72-78-2
2,4-Dinitrotoluene	2,4-DNT	121-14-2
2,6-Dinitrotoluene	2,6-DNT	606-20-2
2-Nitrotoluene	2-NT	88-72-2
3-Nitrotoluene	3-NT	99-08-1
4-Nitrotoluene	4-NT	99-99-0

a Chemical Abstracts Service Registry number

1.2 Method 8330 provides a salting-out extraction procedure for low concentration (parts per trillion, or nanograms per liter) of explosives residues in surface or ground water. Direct injection of diluted and filtered water samples can be used for water samples of higher concentration (See Table 1).

1.3 All of these compounds are either used in the manufacture of explosives or are the degradation products of compounds used for that purpose. When making stock solutions for calibration, treat each explosive compound with caution. See NOTE in Sec. 5.3.1 and Sec. 11 on Safety.

1.4 The estimated quantitation limits (EQLs) of target analytes determined by Method 8330 in water and soil are presented in Table 1.

1.5 This method is restricted to use by or under the supervision of analysts experienced in the use of HPLC, skilled in the interpretation of

chromatograms, and experienced in handling explosive materials. (See Sec. 11.0 on SAFETY.) Each analyst must demonstrate the ability to generate acceptable results with this method.

2.0 SUMMARY OF METHOD

2.1 Method 8330 provides high performance liquid chromatographic (HPLC) conditions for the detection of ppb levels of certain explosives residues in water, soil and sediment matrix. Prior to use of this method, appropriate sample preparation techniques must be used.

2.2 Low-Level Salting-out Method With No Evaporation: Aqueous samples of low concentration are extracted by a salting-out extraction procedure with acetonitrile and sodium chloride. The small volume of acetonitrile that remains undissolved above the salt water is drawn off and transferred to a smaller volumetric flask. It is back-extracted by vigorous stirring with a specific volume of salt water. After equilibration, the phases are allowed to separate and the small volume of acetonitrile residing in the narrow neck of the volumetric flask is removed using a Pasteur pipet. The concentrated extract is diluted 1:1 with reagent grade water. An aliquot is separated on a C-18 reverse phase column, determined at 254 nm, and confirmed on a CN reverse phase column.

2.3 High-level Direct Injection Method: Aqueous samples of higher concentration can be diluted 1/1 (v/v) with methanol or acetonitrile, filtered, separated on a C-18 reverse phase column, determine at 254 nm, and confirmed on a CN reverse phase column. If HMX is an important target analyte, methanol is preferred.

2.4 Soil and sediment samples are extracted using acetonitrile in an ultrasonic bath, filtered and chromatographed as in Sec. 2.3.

3.0 INTERFERENCES

3.1 Solvents, reagents, glassware and other sample processing hardware may yield discrete artifacts and/or elevated baselines, causing misinterpretation of the chromatograms. All of these materials must be demonstrated to be free from interferences.

3.2 2,4-DNT and 2,6-DNT elute at similar retention times (retention time difference of 0.2 minutes). A large concentration of one isomer may mask the response of the other isomer. If it is not apparent that both isomers are present (or are not detected), an isomeric mixture should be reported.

3.3 Tetryl decomposes rapidly in methanol/water solutions, as well as with heat. All aqueous samples expected to contain tetryl should be diluted with acetonitrile prior to filtration and acidified to pH <3. All samples expected to contain tetryl should not be exposed to temperatures above room temperature.

3.4 Degradation products of tetryl appear as a shoulder on the 2,4,6-TNT peak. Peak heights rather than peak areas should be used when tetryl is present in concentrations that are significant relative to the concentration of 2,4,6-TNT.

4.0 APPARATUS AND MATERIALS

4.1 HPLC system

4.1.1 HPLC - equipped with a pump capable of achieving 4000 psi, a 100 μ l loop injector and a 254 nm UV detector (Perkin Elmer Series 3, or equivalent). For the low concentration option, the detector must be capable of a stable baseline at 0.001 absorbance units full scale.

4.1.2 Recommended Columns:

4.1.2.1 Primary column: C-18 Reverse phase HPLC column, 25 cm x 4.6 mm (5 μ m), (Supelco LC-18, or equivalent).

4.1.2.2 Secondary column: CN Reverse phase HPLC column, 25 cm x 4.6 mm (5 μ m), (Supelco LC-CN, or equivalent).

4.1.3 Strip chart recorder.

4.1.4 Digital integrator (optional).

4.1.5 Autosampler (optional).

4.2 Other Equipment

4.2.1 Temperature controlled ultrasonic bath.

4.2.2 Vortex mixer.

4.2.3 Balance, \pm 0.0001 g.

4.2.4 Magnetic stirrer with stirring pellets.

4.2.5 Water bath - Heated, with concentric ring cover, capable of temperature control (\pm 5°C). The bath should be used in a hood.

4.2.6 Oven - Forced air, without heating.

4.3 Materials

4.3.1 High pressure injection syringe - 500 μ L, (Hamilton liquid syringe or equivalent).

4.3.2 Disposable cartridge filters - 0.45 μ m Teflon filter.

4.3.3 Pipets - Class A, glass, Appropriate sizes.

4.3.4 Pasteur pipets.

4.3.5 Scintillation Vials - 20 mL, glass.

4.3.6 Vials - 15 mL, glass, Teflon-lined cap.

4.3.7 Vials- 40 mL, glass, Teflon-lined cap.

4.3.8 Disposable syringes - Plastipak, 3 mL and 10 mL or equivalent.

4.3.9 Volumetric flasks - Appropriate sizes with ground glass stoppers, Class A.

NOTE: The 100 mL and 1 L volumetric flasks used for magnetic stirrer extraction must be round.

4.3.10 Vacuum desiccator - Glass.

4.3.11 Mortar and pestle - Steel.

4.3.12 Sieve - 30 mesh.

4.3.13 Graduated cylinders - Appropriate sizes.

4.4 Preparation of Materials

4.4.1 Prepare all materials to be used as described in Chapter 4 for semivolatile organics.

5.0 REAGENTS

5.1 Reagent grade inorganic chemicals shall be used in all tests. Unless otherwise indicated, it is intended that all reagents shall conform to the specifications of the Committee on Analytical Reagents of the American Chemical Society, where such specifications are available. Other grades may be used, provided it is first ascertained that the reagent is of sufficiently high purity to permit its use without lowering the accuracy of the determination.

5.1.1 Acetonitrile, CH_3CN - HPLC grade.

5.1.2 Methanol, CH_3OH - HPLC grade.

5.1.3 Calcium chloride, CaCl_2 - Reagent grade. Prepare an aqueous solution of 5 g/L.

5.1.4 Sodium chloride, NaCl , shipped in glass bottles - reagent grade.

5.2 Organic-free reagent water - All references to water in this method refer to organic-free reagent water, as defined in Chapter One.

5.3 Stock Standard Solutions

5.3.1 Dry each solid analyte standard to constant weight in a vacuum desiccator in the dark. Place about 0.100 g (weighed to 0.0001 g) of a single analyte into a 100 mL volumetric flask and dilute to volume with

acetonitrile. Invert flask several times until dissolved. Store in refrigerator at 4°C in the dark. Calculate the concentration of the stock solution from the actual weight used (nominal concentration = 1,000 mg/L). Stock solutions may be used for up to one year.

NOTE: The HMX, RDX, Tetryl, and 2,4,6-TNT are explosives and the neat material should be handled carefully. See SAFETY in Sec. 11 for guidance. HMX, RDX, and Tetryl reference materials are shipped under water. Drying at ambient temperature requires several days. DO NOT DRY AT HEATED TEMPERATURES!

5.4 Intermediate Standards Solutions

5.4.1 If both 2,4-DNT and 2,6-DNT are to be determined, prepare two separate intermediate stock solutions containing (1) HMX, RDX, 1,3,5-TNB, 1,3-DNB, NB, 2,4,6-TNT, and 2,4-DNT and (2) Tetryl, 2,6-DNT, 2-NT, 3-NT, and 4-NT. Intermediate stock standard solutions should be prepared at 1,000 µg/L, in acetonitrile when analyzing soil samples, and in methanol when analyzing aqueous samples.

5.4.2 Dilute the two concentrated intermediate stock solutions, with the appropriate solvent, to prepare intermediate standard solutions that cover the range of 2.5 - 1,000 µg/L. These solutions should be refrigerated on preparation, and may be used for 30 days.

5.4.3 For the low-level method, the analyst must conduct a detection limit study and devise dilution series appropriate to the desired range. Standards for the low level method must be prepared immediately prior to use.

5.5 Working standards

5.5.1 Calibration standards at a minimum of five concentration levels should be prepared through dilution of the intermediate standards solutions by 50% (v/v) with 5 g/L calcium chloride solution (Sec. 5.1.3). These solutions must be refrigerated and stored in the dark, and prepared fresh on the day of calibration.

5.6 Surrogate Spiking Solution

5.6.1 The analyst should monitor the performance of the extraction and analytical system as well as the effectiveness of the method in dealing with each sample matrix by spiking each sample, standard and reagent water blank with one or two surrogates (e.g., analytes not expected to be present in the sample).

5.7 Matrix Spiking Solutions

5.7.1 Prepare matrix spiking solutions in methanol such that the concentration in the sample is five times the Estimated Quantitation Limit (Table 1). All target analytes should be included.

5.8 HPLC Mobile Phase

5.8.1 To prepare 1 liter of mobile phase, add 500 mL of methanol to 500 mL of organic-free reagent water.

6.0 SAMPLE COLLECTION, PRESERVATION, AND HANDLING

6.1 Follow conventional sampling and sample handling procedures as specified for semivolatile organics in Chapter Four.

6.2 Samples and sample extracts must be stored in the dark at 4°C. Holding times are the same as for semivolatile organics.

7.0 PROCEDURE

7.1 Sample Preparation

7.1.1 Aqueous Samples: It is highly recommended that process waste samples be screened with the high-level method to determine if the low level method (1-50 µg/L) is required. Most groundwater samples will fall into the low level method.

7.1.1.1 Low-Level Method (salting-out extraction)

7.1.1.1.1 Add 251.3 g of sodium chloride to a 1 L volumetric flask (round). Measure out 770 mL of a water sample (using a 1 L graduated cylinder) and transfer it to the volumetric flask containing the salt. Add a stir bar and mix the contents at maximum speed on a magnetic stirrer until the salt is completely dissolved.

7.1.1.1.2 Add 164 mL of acetonitrile (measured with a 250 mL graduated cylinder) while the solution is being stirred and stir for an additional 15 minutes. Turn off the stirrer and allow the phases to separate for 10 minutes.

7.1.1.1.3 Remove the acetonitrile (upper) layer (about 8 mL) with a Pasteur pipet and transfer it to a 100 mL volumetric flask (round). Add 10 mL of fresh acetonitrile to the water sample in the 1 L flask. Again stir the contents of the flask for 15 minutes followed by 10 minutes for phase separation. Combine the second acetonitrile portion with the initial extract. The inclusion of a few drops of salt water at this point is unimportant.

7.1.1.1.4 Add 84 mL of salt water (325 g NaCl per 1000 mL of reagent water) to the acetonitrile extract in the 100 mL volumetric flask. Add a stir bar and stir the contents on a magnetic stirrer for 15 minutes, followed by 10 minutes for phase separation. Carefully transfer the acetonitrile phase

to a 10 mL graduated cylinder using a Pasteur pipet. At this stage, the amount of water transferred with the acetonitrile must be minimized. The water contains a high concentration of NaCl that produces a large peak at the beginning of the chromatogram, where it could interfere with the HMX determination.

7.1.1.1.5 Add an additional 1.0 mL of acetonitrile to the 100 mL volumetric flask. Again stir the contents of the flask for 15 minutes, followed by 10 minutes for phase separation. Combine the second acetonitrile portion with the initial extract in the 10 mL graduated cylinder (transfer to a 25 mL graduated cylinder if the volume exceeds 5 mL). Record the total volume of acetonitrile extract to the nearest 0.1 mL. (Use this as the volume of total extract [V_t] in the calculation of concentration after converting to μL). The resulting extract, about 5 - 6 mL, is then diluted 1:1 with organic-free reagent water (with pH <3 if tetryl is a suspected analyte) prior to analysis.

7.1.1.1.6 If the diluted extract is turbid, filter it through a 0.45 - μm Teflon filter using a disposable syringe. Discard the first 0.5 mL of filtrate, and retain the remainder in a Teflon-capped vial for RP-HPLC analysis as in Sec. 7.4.

7.1.1.2 High-Level Method

7.1.1.2.1 Sample filtration: Place a 5 mL aliquot of each water sample in a scintillation vial, add 5 mL of acetonitrile, shake thoroughly, and filter through a 0.45- μm Teflon filter using a disposable syringe. Discard the first 3 mL of filtrate, and retain the remainder in a Teflon-capped vial for RP-HPLC analysis as in Sec. 7.4. HMX quantitation can be improved with the use of methanol rather than acetonitrile for dilution before filtration.

7.1.2 Soil and Sediment Samples

7.1.2.1 Sample homogenization: Dry soil samples in air at room temperature or colder to a constant weight, being careful not to expose the samples to direct sunlight. Grind and homogenize the dried sample thoroughly in an acetonitrile-rinsed mortar to pass a 30 mesh sieve.

NOTE: Soil samples should be screened by Method 8515 prior to grinding in a mortar and pestle (See Safety Sec. 11.2).

7.1.2.2 Sample extraction

7.1.2.2.1 Place a 2.0 g subsample of each soil sample in a 15 mL glass vial. Add 10.0 mL of acetonitrile, cap with

Teflon-lined cap, vortex swirl for one minute, and place in a cooled ultrasonic bath for 18 hours.

7.1.2.2.2 After sonication, allow sample to settle for 30 minutes. Remove 5.0 mL of supernatant, and combine with 5.0 mL of calcium chloride solution (Sec. 5.1.3) in a 20 mL vial. Shake, and let stand for 15 minutes.

7.1.2.2.3 Place supernatant in a disposable syringe and filter through a 0.45- μ m Teflon filter. Discard first 3 mL and retain remainder in a Teflon-capped vial for RP-HPLC analysis as in Sec. 7.4.

7.2 Chromatographic Conditions (Recommended)

Primary Column: C-18 reverse phase HPLC column, 25-cm x 4.6-mm, 5 μ m, (Supelco LC-18 or equivalent).

Secondary Column: CN reverse phase HPLC column, 25-cm x 4.6-mm, 5 μ m, (Supelco LC-CN or equivalent).

Mobile Phase: 50/50 (v/v) methanol/organic-free reagent water.

Flow Rate: 1.5 mL/min

Injection volume: 100- μ L

UV Detector: 254 nm

7.3 Calibration of HPLC

7.3.1 All electronic equipment is allowed to warm up for 30 minutes. During this period, at least 15 void volumes of mobile phase are passed through the column (approximately 20 min at 1.5 mL/min) and continued until the baseline is level at the UV detector's greatest sensitivity.

7.3.2 Initial Calibration. Injections of each calibration standard over the concentration range of interest are made sequentially into the HPLC in random order. Peak heights or peak areas are obtained for each analyte. Experience indicates that a linear calibration curve with zero intercept is appropriate for each analyte. Therefore, a response factor for each analyte can be taken as the slope of the best-fit regression line.

7.3.3 Daily Calibration. Analyze midpoint calibration standards, at a minimum, at the beginning of the day, singly at the midpoint of the run, and singly after the last sample of the day (assuming a sample group of 10 samples or less). Obtain the response factor for each analyte from the mean peak heights or peak areas and compare it with the response factor obtained for the initial calibration. The mean response factor for the

daily calibration must agree within $\pm 15\%$ of the response factor of the initial calibration. The same criteria is required for subsequent standard responses compared to the mean response of the triplicate standards beginning the day. If this criterion is not met, a new initial calibration must be obtained.

7.4 HPLC Analysis

7.4.1 Analyze the samples using the chromatographic conditions given in Sec. 7.2. All positive measurements observed on the C-18 column must be confirmed by injection onto the CN column.

7.4.2 Follow Sec. 7.0 in Method 8000 for instructions on the analysis sequence, appropriate dilutions, establishing daily retention time windows, and identification criteria. Include a mid-level standard after each group of 10 samples in the analysis sequence. If column temperature control is not employed, special care must be taken to ensure that temperature shifts do not cause peak misidentification.

7.4.3 Table 2 summarizes the estimated retention times on both C-18 and CN columns for a number of analytes analyzable using this method. An example of the separation achieved by Column 1 is shown in Figure 1.

7.4.4 Record the resulting peak sizes in peak heights or area units. The use of peak heights is recommended to improve reproducibility of low level samples.

7.4.5 Calculation of concentration is covered in Sec. 7.0 of Method 8000.

8.0 QUALITY CONTROL

8.1 Refer to Chapter One for specific quality control procedures. Quality control to validate sample extraction is covered in Method 3500.

8.2 Quality control required to validate the HPLC system operation is found in Method 8000, Sec. 8.0.

8.3 Prior to preparation of stock solutions, acetonitrile, methanol, and water blanks should be run to determine possible interferences with analyte peaks. If the acetonitrile, methanol, or water blanks show contamination, a different batch should be used.

9.0 METHOD PERFORMANCE

9.1 Table 3 presents the single laboratory precision based on data from the analysis of blind duplicates of four spiked soil samples and four field contaminated samples analyzed by seven laboratories.

9.2 Table 4 presents the multilaboratory error based on data from the analysis of blind duplicates of four spiked soil samples and four field contaminated samples analyzed by seven laboratories.

9.3 Table 5 presents the multilaboratory variance of the high concentration method for water based on data from nine laboratories.

9.4 Table 6 presents multilaboratory recovery data from the analysis of spiked soil samples by seven laboratories.

9.5 Table 7 presents a comparison of method accuracy for soil and aqueous samples (high concentration method).

9.6 Table 8 contains precision and accuracy data for the salting-out extraction method.

10.0 REFERENCES

1. Bauer, C.F., T.F. Jenkins, S.M. Koza, P.W. Schumacher, P.H. Miyares and M.E. Walsh (1989). Development of an analytical method for the determination of explosive residues in soil. Part 3. Collaborative test results and final performance evaluation. USA Cold Regions Research and Engineering Laboratory, CRREL Report 89-9.
2. Grant, C.L., A.D. Hewitt and T.F. Jenkins (1989) Comparison of low concentration measurement capability estimates in trace analysis: Method Detection Limits and Certified Reporting Limits. USA Cold Regions Research and Engineering Laboratory, Special Report 89-20.
3. Jenkins, T.F., C.F. Bauer, D.C. Leggett and C.L. Grant (1984) Reversed-phased HPLC method for analysis of TNT, RDX, HMX and 2,4-DNT in munitions wastewater. USA Cold Regions Research and Engineering Laboratory, CRREL Report 84-29.
4. Jenkins, T.F. and M.E. Walsh (1987) Development of an analytical method for explosive residues in soil. USA Cold Regions Research and Engineering Laboratory, CRREL Report 87-7.
5. Jenkins, T.F., P.H. Miyares and M.E. Walsh (1988a) An improved RP-HPLC method for determining nitroaromatics and nitramines in water. USA Cold Regions Research and Engineering Laboratory, Special Report 88-23.
6. Jenkins, T.F. and P.H. Miyares (1992) Comparison of Cartridge and Membrane Solid-Phase Extraction with Salting-out Solvent Extraction for Preconcentration of Nitroaromatic and Nitramine Explosives from Water. USA Cold Regions Research and Engineering Laboratory, Draft CRREL Special Report.
7. Jenkins, T.F., P.W. Schumacher, M.E. Walsh and C.F. Bauer (1988b) Development of an analytical method for the determination of explosive

residues in soil. Part II: Further development and ruggedness testing. USA Cold Regions Research and Engineering Laboratory, CRREL Report 88-8.

8. Leggett, D.C., T.F. Jenkins and P.H. Miyares (1990) Salting-out solvent extraction for preconcentration of neutral polar organic solutes from water. *Analytical Chemistry*, 62: 1355-1356.
9. Miyares, P.H. and T.F. Jenkins (1990) Salting-out solvent extraction for determining low levels of nitroaromatics and nitramines in water. USA Cold Regions Research and Engineering Laboratory, Special Report 90-30.

11.0 SAFETY

11.1 Standard precautionary measures used for handling other organic compounds should be sufficient for the safe handling of the analytes targeted by Method 8330. The only extra caution that should be taken is when handling the analytical standard neat material for the explosives themselves and in rare cases where soil or waste samples are highly contaminated with the explosives. Follow the note for drying the neat materials at ambient temperatures.

11.2 It is advisable to screen soil or waste samples using Method 8515 to determine whether high concentrations of explosives are present. Soil samples as high as 2% 2,4,6-TNT have been safely ground. Samples containing higher concentrations should not be ground in the mortar and pestle. Method 8515 is for 2,4,6-TNT, however, the other nitroaromatics will also cause a color to be developed and provide a rough estimation of their concentrations. 2,4,6-TNT is the analyte most often detected in high concentrations in soil samples. Visual observation of a soil sample is also important when the sample is taken from a site expected to contain explosives. Lumps of material that have a chemical appearance should be suspect and not ground. Explosives are generally a very finely ground grayish-white material.

TABLE 1
ESTIMATED QUANTITATION LIMITS

Compounds	Water ($\mu\text{g/L}$)		Soil (mg/kg)
	Low-Level	High-Level	
HMX	-	13.0	2.2
RDX	0.84	14.0	1.0
1,3,5-TNB	0.26	7.3	0.25
1,3-DNB	0.11	4.0	0.25
Tetryl	-	4.0	0.65
NB	-	6.4	0.26
2,4,6-TNT	0.11	6.9	0.25
4-Am-DNT	0.060	-	-
2-Am-DNT	0.035	-	-
2,6-DNT	0.31	9.4	0.26
2,4-DNT	0.020	5.7	0.25
2-NT	-	12.0	0.25
4-NT	-	8.5	0.25
3-NT	-	7.9	0.25

TABLE 2
RETENTION TIMES AND CAPACITY FACTORS ON LC-18 AND LC-CN COLUMNS

Compound	Retention time (min)		Capacity factor (k)*	
	LC-18	LC-CN	LC-18	LC-CN
HMX	2.44	8.35	0.49	2.52
RDX	3.73	6.15	1.27	1.59
1,3,5-TNB	5.11	4.05	2.12	0.71
1,3-DNB	6.16	4.18	2.76	0.76
Tetryl	6.93	7.36	3.23	2.11
NB	7.23	3.81	3.41	0.61
2,4,6-TNT	8.42	5.00	4.13	1.11
4-Am-DNT	8.88	5.10	4.41	1.15
2-Am-DNT	9.12	5.65	4.56	1.38
2,6-DNT	9.82	4.61	4.99	0.95
2,4-DNT	10.05	4.87	5.13	1.05
2-NT	12.26	4.37	6.48	0.84
4-NT	13.26	4.41	7.09	0.86
3-NT	14.23	4.45	7.68	0.88

* Capacity factors are based on an unretained peak for nitrate at 1.71 min on LC-18 and at 2.00 min on LC-CN.

TABLE 3
SINGLE LABORATORY PRECISION OF METHOD FOR SOIL SAMPLES

	Spiked Soils			Field-Contaminated Soils		
	Mean Conc. (mg/kg)	SD	%RSD	Mean Conc. (mg/kg)	SD	%RSD
HMX	46	1.7	3.7	14	1.8	12.8
				153	21.6	14.1
RDX	60	1.4	2.3	104	12	11.5
				877	29.6	3.4
1,3,5-TNB	8.6	0.4	4.6	2.8	0.2	7.1
	46	1.9	4.1	72	6.0	8.3
1,3-DNB	3.5	0.14	4.0	1.1	0.11	9.8
Tetryl	17	3.1	17.9	2.3	0.41	18.0
2,4,6-TNT	40	1.4	3.5	7.0	0.61	9.0
				669	55	8.2
2,4-DNT	5.0	0.17	3.4	1.0	0.44	42.3

TABLE 4
MULTILABORATORY ERROR OF METHOD FOR SOIL SAMPLES

	Spiked Soils			Field-Contaminated Soils		
	Mean Conc. (mg/kg)	SD	%RSD	Mean Conc. (mg/kg)	SD	%RSD
HMX	46	2.6	5.7	14	3.7	26.0
				153	37.3	24.0
RDX	60	2.6	4.4	104	17.4	17.0
				877	67.3	7.7
1,3,5-TNB	8.6	0.61	7.1	2.8	0.23	8.2
	46	2.97	6.5	72	8.8	12.2
1,3-DNB	3.5	0.24	6.9	1.1	0.16	14.5
Tetryl	17	5.22	30.7	2.3	0.49	21.3
2,4,6-TNT	40	1.88	4.7	7.0	1.27	18.0
				669	63.4	9.5
2,4-DNT	5.0	0.22	4.4	1.0	0.74	74.0

TABLE 5
MULTILABORATORY VARIANCE OF METHOD FOR WATER SAMPLES^a

Compounds	Mean Conc. (µg/L)	SD	%RSD
HMX	203	14.8	7.3
RDX	274	20.8	7.6
2,4-DNT	107	7.7	7.2
2,4,6-TNT	107	11.1	10.4

^a Nine Laboratories

TABLE 6
MULTILABORATORY RECOVERY DATA FOR SPIKED SOIL SAMPLES

Laboratory	Concentration ($\mu\text{g/g}$)						
	HMX	RDX	1,3,5-TNB	1,3-DNB	Tetryl	2,4,6-TNT	2,4-DNT
1	44.97	48.78	48.99	49.94	32.48	49.73	51.05
3	50.25	48.50	45.85	45.96	47.91	46.25	48.37
4	42.40	44.00	43.40	49.50	31.60	53.50	50.90
5	46.50	48.40	46.90	48.80	32.10	55.80	49.60
6	56.20	55.00	41.60	46.30	13.20	56.80	45.70
7	41.50	41.50	38.00	44.50	2.60	36.00	43.50
8	52.70	52.20	48.00	48.30	44.80	51.30	49.10
True Conc	50.35	50.20	50.15	50.05	50.35	50.65	50.05
Mean	47.79	48.34	44.68	47.67	29.24	49.91	48.32
Std Dev	5.46	4.57	3.91	2.09	16.24	7.11	2.78
% RSD	11.42	9.45	8.75	4.39	55.53	14.26	5.76
% Diff*	5.08	3.71	10.91	4.76	41.93	1.46	3.46
Mean % Recovery	95	96	89	95	58	98	96

* Between true value and mean determined value.

TABLE 7
 COMPARISON OF METHOD ACCURACY FOR SOIL AND AQUEOUS SAMPLES
 (HIGH CONCENTRATION METHOD)

Analyte	Recovery (%)	
	Soil Method*	Aqueous Method**
2,4-DNT	96.0	98.6
2,4,6-TNT	96.8	94.4
RDX	96.8	99.6
HMX	95.4	95.5

* Taken from Bauer et al. (1989), Reference 1.


** Taken from Jenkins et al. (1984), Reference 3.

TABLE 8
PRECISION AND ACCURACY DATA FOR THE SALTING-OUT EXTRACTION METHOD

Analyte	No. of Samples ¹	Precision (% RSD)	Ave. Recovery (%)	Conc. Range (µg/L)
HMX	20	10.5	106	0-1.14
RDX	20	8.7	106	0-1.04
1,3,5-TNB	20	7.6	119	0-0.82
1,3-DNB	20	6.6	102	0-1.04
Tetryl	20	16.4	93	0-0.93
2,4,6-TNT	20	7.6	105	0-0.98
2-Am-DNT	20	9.1	102	0-1.04
2,4-DNT	20	5.8	101	0-1.01
1,2-NT	20	9.1	102	0-1.07
1,4-NT	20	18.1	96	0-1.06
1,3-NT	20	12.4	97	0-1.23

¹Reagent water

**EXPLOSIVES ON A
C18 COLUMN**

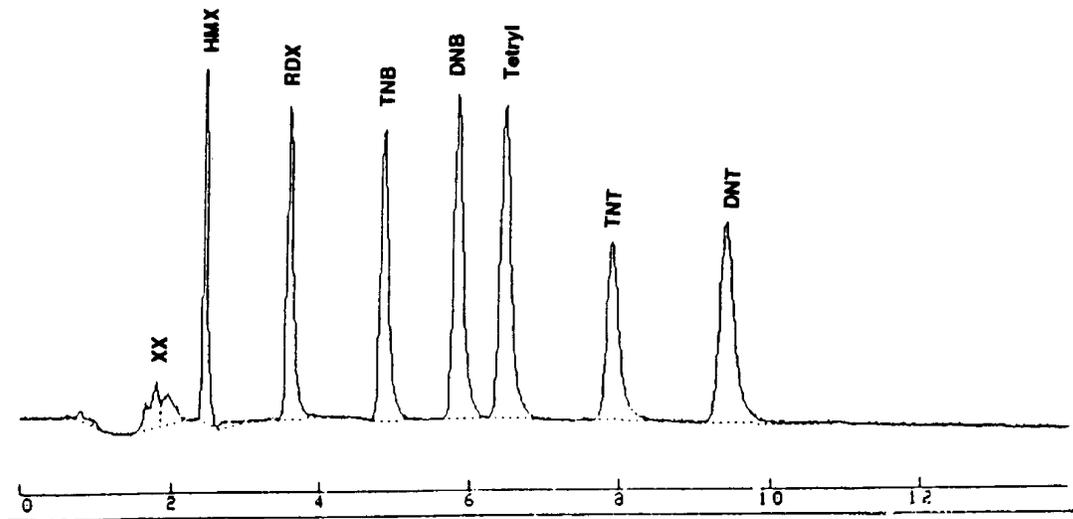

**EXPLOSIVES ON A
CN COLUMN**

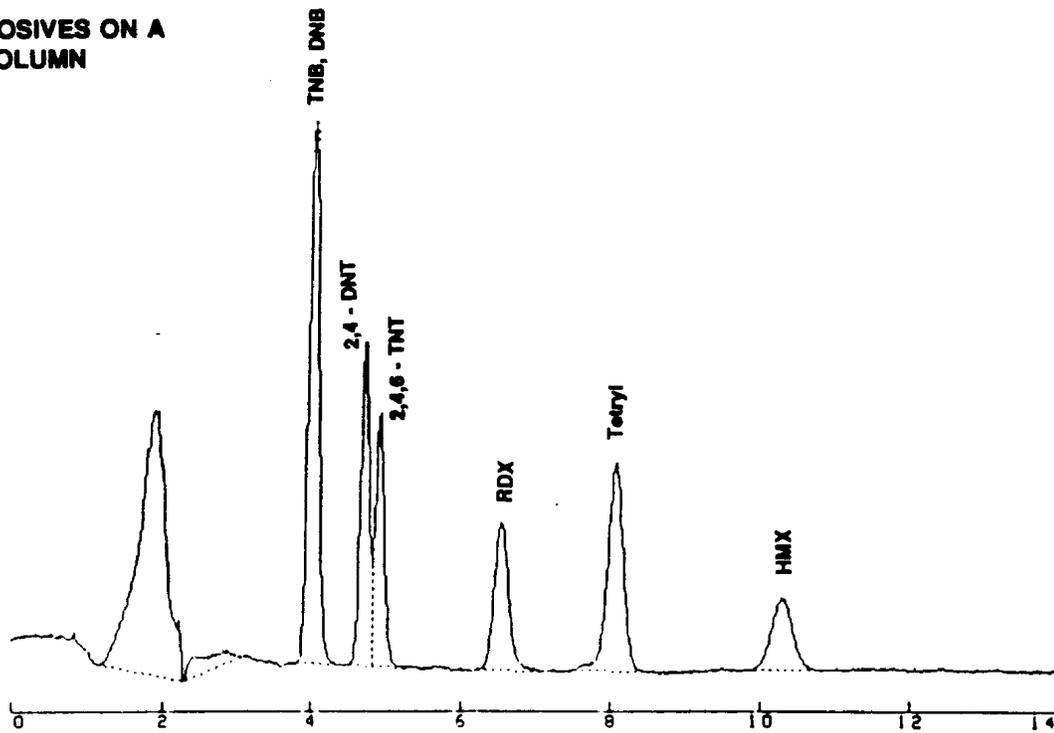


FIGURE 1
CHROMATOGRAMS FOR COLUMNS DESCRIBED IN Sec. 4.1.2.
COURTESY OF U.S. ARMY CORPS OF ENGINEERS, OMAHA, NE.

METHOD 8330
NITROAROMATICS AND NITRAMINES BY HIGH
PERFORMANCE LIQUID CHROMATOGRAPHY (HPLC)

